

Recombinant multi-epitope chimeric antigen ChimToxo1 for *Toxoplasma gondii*

CATALOG NUMBER: RAG0058

LOT NUMBER: #

RECOMBINANT ANTIGEN: recombinant multi-epitope chimeric antigen for *T. gondii*

DESCRIPTION: the recombinant multi-epitope chimeric antigen of Toxo has been prepared as a chimeric protein formed by some antigenic determinants of SAG1 and GRA8 of this parasite.

PRESENTATION: liquid protein solution

SOURCE: *Pichia pastoris*

SPECIFIC ANTIBODY (CALIBRATOR): IgG polyclonal antibody against GRA7 and GRA8 (Rekom Biotech catalog reference PAB0005)

MOLECULAR WEIGHT: SDS-PAGE analysis determines that the protein band is between the molecular markers of 66,000 Da and 45,000 Da due to the glycosylation pattern, while relative molecular mass, calculated from amino acid sequence and without glycosylation, is 38,636.97 Da.

BATCH COMPOSITION:

COMPONENTS	COMPOSITION
his-ChimToxo1	recombinant chimeric antigen with a his-tag in its N-terminus
Storage buffer	20 mM phosphate buffer pH 7 and 0.1 M KCl

QUALITY CONTROL:

1. PROTEIN CONCENTRATION DETERMINED ESPECTROPHOTOMETRICALLY

$DO_{280} = 1.054$

$A_{0.1\%} (=1 \text{ g/l}) = 0.719$

CONCENTRATION*: 1.47 mg/ml

* The measurement of the protein concentration has been performed with the theoretical extinction coefficient of the recombinant protein obtained from Gill and von Hippel, 1989. It is recommended that the users carry out their absorbance determinations to avoid equipment variabilities regarding final concentration, mainly in reproducibility analysis.

2. PURITY CONTROL IN SDS-PAGE: 15%

kDa Mw ChimToxo1

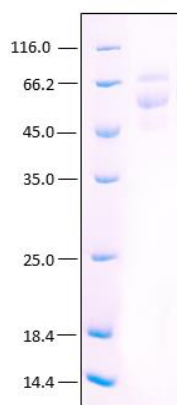


Figure 1. SDS-PAGE analysis (15%) of 4 µl of recombinant ChimToxo1. Purity is >95% as determined by gel electrophoresis. Both bands correspond to the target protein as react with an anti-His Ab.

3. DISCRIMINATION OF PRE-VALIDATED SERA BY AN INDIRECT ELISA ASSAY

The cut-off has been suggested about an "in-house" ELISA kit performed in Rekom Biotech.

Each end-user should carry out an analysis for their particular application.

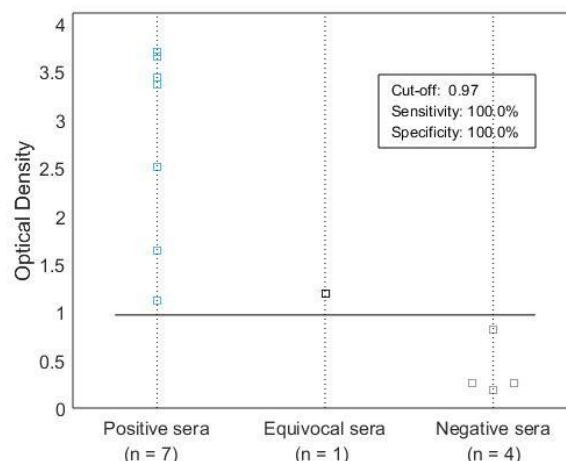


Figure 2. The dot plot graph illustrates the distribution of positive and negative sera by an indirect IgG ELISA with a ChimToxo1 plate coating of 1 µg/ml. Pre-validated sera by Dx (IgG, LIAISON, Diasorin, CLIA) were used in this analysis. The chart shows the optical density at 450/620 nm for positive (blue) and negative (grey) IgG sera. **For specimen discrimination sera, 8 µg of anti-CCD blocker (Ref. Rekom SOR0001, see COA) was added to the sera 10 min before incubation with the coated antigen.**

4. WESTERN BLOT ANALYSIS

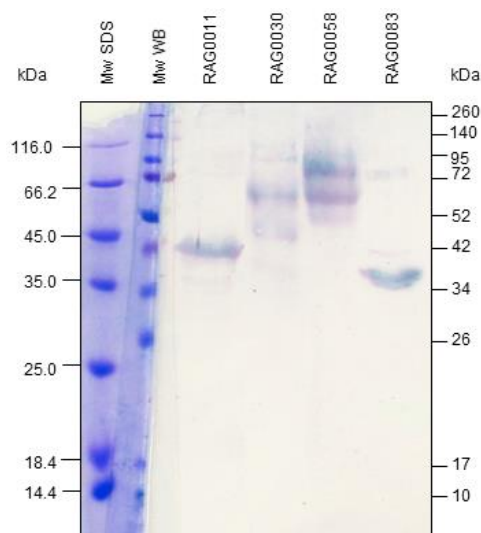


Figure 3. When a polyclonal Ab obtained by using a clarified native extract of sporozoite oocysts of *Toxoplasma gondii* as immunogen was used in a western blot analysis, clear signals were obtained in our recombinant antigens for *T. gondii* RAG0030, RAG0011, RAG0083 and RAG0058.

5. ABSENCE OF PRECIPITATION AFTER A FREEZING AND THAWING CYCLE: ok

LOT SPECIFICATIONS:

1. CONCENTRATION: 1.47 mg/ml

2. TOTAL QUANTITY PER ALIQUOT: 1 mg

3. TOTAL VOLUME PER ALIQUOT: 0.714 ml

4. SUGGESTED TITER BY ELISA: up to 1:1,470, which corresponds to 1 µg/ml of protein concentration in plates for IgG detection in an indirect ELISA assay.

5. STORAGE: Protein is shipped with dry ice. Upon arrival, it should be aliquoted to avoid repeated freezing and thawing cycles and stored at -20°C to -80°C. In order to defrost the protein, maintain the aliquot at 25°C without shaking to avoid aggregation.

6. TESTED APPLICATIONS: ELISA and western blot.

7. POSSIBLE APPLICATIONS: WB, DB, Indirect ELISA, positive control in direct ELISA, CLIA, lateral-flow. Where this product has not been tested for use in a particular technique, this does not necessarily exclude its use in such procedures. Suggested working dilutions are given as a guide only. It is recommended that the user titrates. **Due to the nonspecific interaction with anti-CCDs present in normal human or animal sera, we strongly recommend using our blocker SOR0001 on the analyzed sera in any immunoassay.**

8. OBSERVATIONS: proteins should be maintained frozen at high concentrations. The dilution to be performed for ELISA assays should be made with a small quantity of protein, the same day of the experiment. In order to defrost the protein, maintain the aliquot at 25°C without shaking to avoid aggregation. Prior making test dilutions and after defrosting the protein, is recommended to remove possible protein aggregates by centrifuging the stock solution, avoiding alterations in the immobilization of the biomolecule to the solid surface.

RELATED PRODUCTS:

p29 (GRA7), p30 (SAG1), p35 (GRA8).

BIBLIOGRAPHY:

Santoro, F., Charif, H. and Capron, A. The immunodominant epitope of the major membrane tachyzoite protein (p30) of *Toxoplasma gondii*. 1986, *Parasite Immunol.* 8:631-9.

Gill SC, von Hippel PH. Calculation of protein extinction coefficients from amino acid sequence data. *Anal Biochem.* 1989 Nov 1;182(2):319-26.

CEO Signature:
Date: 25/06/2020



Important Notes: During shipment, small volumes of product will occasionally become entrapped in the seal of the product vial. For products with volumes of 200 µl or less, we recommend gently tapping the vial on a hard surface or briefly centrifuging the vial in a tabletop centrifuge to dislodge any liquid in the containers cap.

Although recombinant antigens are expressed in non-pathogenic *P. pastoris* and bacterial integrity is destroyed during purification, the antigen preparation should be handled as potentially infectious.

FOR RESEARCH AND COMMERCIAL USE *IN VITRO*: not for human *in vivo* or therapeutic use.