

Recombinant biotinylated chimeric antigen ChimChagas3 for *Trypanosoma cruzi*

CATALOG NUMBER: RAG0096BIOT

LOT NUMBER: #

RECOMBINANT ANTIGEN: recombinant biotinylated chimeric antigen for Chagas.

DESCRIPTION: the recombinant biotinylated chimeric antigen for Chagas has been prepared as a chimeric protein formed by several antigenic regions from some antigens of this parasite.

PRESENTATION: liquid protein solution

SOURCE: *Escherichia coli*

MOLECULAR WEIGHT: determined by SDS-PAGE, the protein band appears between the molecular markers of 66,200 and 116,000 Da, while relative molecular mass calculated from amino acid sequence is 54,468.89 Da.

BATCH COMPOSITION:

COMPONENTS	COMPOSITION
his-ChimChagas3	recombinant biotinylated chimeric antigen with a his-tag in its N-terminus
Storage buffer	20 mM phosphate buffer pH 8, 0.15 M NaCl and 0.1% polyoxyethylene (10) tridecyl ether

QUALITY CONTROL:

1. PROTEIN CONCENTRATION DETERMINED ESPECTROPHOTOMETRICALLY

DO₂₈₀ = 0.188
 A_{0.1%} (=1 g/l) = 0.163
 CONCENTRATION*: 1.15 mg/ml

* The measurement of the protein concentration has been performed with the theoretical extinction coefficient of the recombinant protein obtained from Gill and vonHippel, 1989. It is recommended that the users carry out their absorbance determinations to avoid equipment variabilities regarding final concentration, mainly in reproducibility analysis.

2. PURITY CONTROL IN SDS-PAGE: 15%

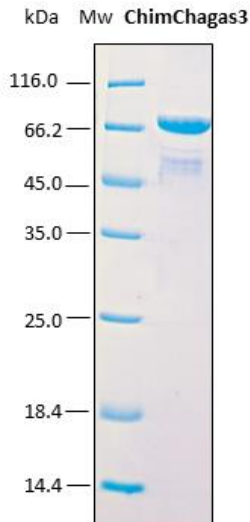


Figure 1. SDS-PAGE analysis (15%) of 3 µl of recombinant biotinylated ChimChagas3. Purity is > 95% as determined by gel electrophoresis.

3. TITRATION CURVE BY AN ELISA ASSAY

The titer has been suggested in reference to an "in-house" ELISA assay performed at Rekom Biotech over the first lot obtained. ELISA assays were performed with a serum sample panel of 25 positive-specimen sera and 5 negative specimen sera, validated by chemiluminescence (Architect, Abbot) and obtained from the Andalusian Public health System Biobank.

Each end user should carry out their own titration for their particular application.

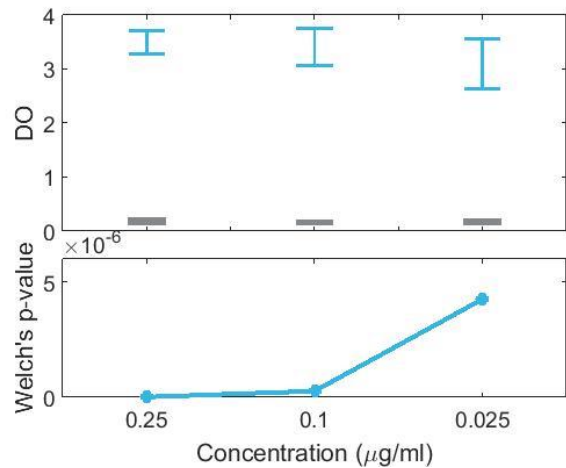


Figure 2. In this plot, the optical density at 450/620 nm for positive (blue) and negative (gray) IgG sera for Chagas disease are compared for each concentration of the recombinant antigen. An appropriate statistical test of significance for the comparison of means between both groups, the Welch's test, is employed. Eligible concentrations for the use of the antigen should present statistically significant differences between positive and negative sera. This happens when the intervals at the top do not overlap and, equivalently, when the p-value at the bottom is below 0.05. In the present figure, all p-values are below 0.05 and thus the intervals do not overlap. Therefore, any of the showed concentrations can be used to distinguish between positive and negative sera.

4. POSITIVE AND NEGATIVE SERA DISCRIMINATION BY AN ELISA ASSAY

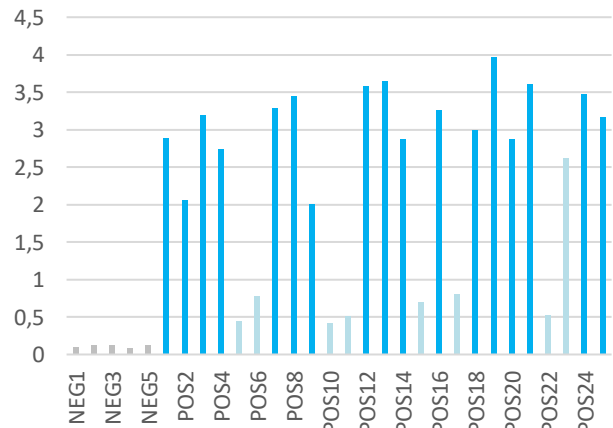


Figure 3. This plot shows an indirect IgG ELISA assay performed with the ChimChagas3 recombinant antigen. the optical density at 450/620 nm for high-positive sera (dark blue), low-positive sera (light blue) and negative sera (gray) are displayed in the graphic.

5. WESTERN BLOT WITH STREPTAVIDIN TO DETECT BIOTINYLATION

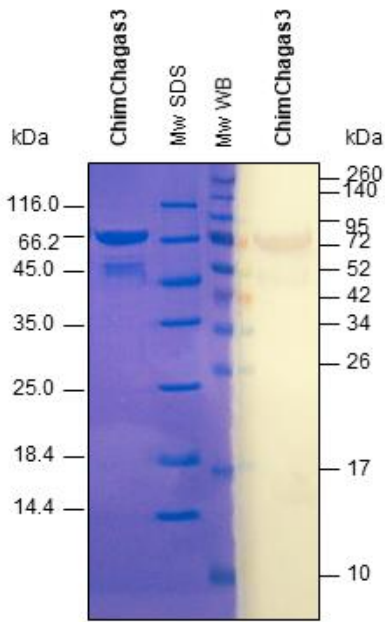


Figure 3. Western blot analysis in order to detect streptavidin/biotin reaction. The incubation was performed with HRP conjugated streptavidin (1:2500)

6. ABSENCE OF PRECIPITATION AFTER A FREEZING AND THAWING CYCLE: ok

LOT SPECIFICATIONS:

- 1. CONCENTRATION:** 1.15 mg/ml
- 2. TOTAL QUANTITY PER ALIQUOT:** 1 mg
- 3. TOTAL VOLUME PER ALIQUOT:** 0.913 ml
- 4. SUGGESTED TITER BY ELISA:** up to 1:46,000, this corresponds to 0.025 µg/ml of protein concentration in plates for IgG detection.
- 5. STORAGE:** Protein is shipped with dry ice. Upon arrival, it should be aliquoted to avoid repeated freezing and thawing cycles and stored at -20°C to -80°C. In order to defrost the protein, maintain the aliquot at 25°C without shaking to avoid aggregation.

Important Notes: During shipment, small volumes of product will occasionally become entrapped in the seal of the product vial. For products with volumes of 200 µl or less, we recommend gently tapping the vial on a hard surface or briefly centrifuging the vial in a tabletop centrifuge to dislodge any liquid in the containers cap.

Although recombinant antigens are expressed in non-pathogenic *E. coli* and bacterial integrity is destroyed during purification, the antigen preparation should be handled as potentially infectious.

FOR RESEARCH AND COMMERCIAL USE *IN VITRO*: not for human *in vivo* or therapeutic use.

6. TESTED APPLICATIONS: ELISA.

7. POSSIBLE APPLICATIONS: WB, DB, Capture ELISA, Double Antigen Sandwich (DAS), nanoparticles binding, plate orientation. Where this product has not been tested for use in a particular technique, this does not necessarily exclude its use in such procedures. Suggested working dilutions are given as a guide only. It is recommended that the user titrates.

8. OBSERVATIONS: in some cases, purified proteins run at a molecular weight which is slightly different to the theoretically calculated molecular weight maybe due to the his-tag presence or sequences of hydrophobic residues, which can produce a delay in SDS-PAGE. Proteins should be maintained frozen at high concentration. The dilution to be performed for carrying out an ELISA assays, should be freshly made with a small quantity of protein. In order to defrost the protein, maintain the aliquot at 25°C without shaking to avoid aggregation. Prior making test dilutions and after defrosting the protein, is recommended to remove possible protein aggregates by centrifuging the stock solution, avoiding alterations in the immobilization of the biomolecule to the solid surface.

RECOMMENDED MATCHED ANTIGEN PAIRS:

CAPTURE: RAG0096
DETECTION: RAG0096BIOT

RELATED PRODUCTS:

1F8, B13, FRA, ChimChagas1, ChimChagas2, ChimChagas3.

BIBLIOGRAPHY:

Gill SC, von Hippel PH. Calculation of protein extinction coefficients from amino acid sequence data. *Anal Biochem.* 1989 Nov 1;182(2):319-26.